

Highlights:

- Qualitative results in less than 2 hours
- Volume packaged (V50)

Contents of Kit:

- 50 96-well Cry2A antibody-coated solid plates
- Cry2A Positive Control
- Cry2A-Enzyme Conjugate
- Substrate

Note: To handle bulk packaged Cry2A-Enzyme Conjugate and Substrate, pour off 5.5 mL of Conjugate and 11.5 mL Substrate per plate to be run each day. Use a multiple-channel pipette to dispense. Do not pour excess Substrate back into the reagent bottle.



Prepare Solutions

Catalog Number AP 005 CT NW V50

Intended Use

The QualiPlate Kit for Cry2A is designed for the non-quantitative laboratory detection of Cry2A endotoxins in corn and cotton leaf and seed tissue.

How the Test Works

This kit is a “sandwich” Enzyme-Linked ImmunoSorbent Assay (ELISA). In the test, plant leaf or seed sample extracts are added to test wells coated with antibodies raised against Cry2A toxin. Any residues present in the sample extract bind to the antibodies, and are then detected by addition of enzyme (horseradish peroxidase)-labeled Cry2A antibody.

After a simple wash step, the results of the assay are visualized with a color development step; color development is proportional to Cry2A concentration in the sample extract.

Lighter color = Lower concentration

Darker color = Higher concentration

Materials Not Provided

- Wash Buffer (preparation instructions below)
- Extraction Buffer (preparation instructions below)
- Stop Solution (preparation instructions below)
- disposable tip, adjustable air-displacement pipettes which will measure 100 microliters (μ L), preferably of multi-channel style
- marking pen (indelible)
- tape or Parafilm®
- timer
- microtiter plate reader or strip reader with 450 nm filter
- wash bottle, or microtiter plate or strip washer
- orbital plate shaker (optional)

Preparation of Solutions


- **Wash Buffer:** 0.01M Phosphate/0.15M Saline/ 0.05% Tween-20 Solution, pH 7.4. This can be purchased in 1L dry packets from Sigma Chemicals, Cat#P-3563, or prepared from salts and Tween-20 on site. Store at controlled ambient temperature for up to one week, then discard.
- **Extraction Buffer:** Prepare Extraction Buffer by adding 0.5 mL Tween-20 to 100 mL of Wash Buffer, for a final solution that is 0.01M Phosphate/ 0.15M Saline/0.55% Tween-20 Solution, pH 7.4.
- 1 N Hydrochloric acid (HCl) **Stop Solution:** Prepare by adding 83 mL of concentrated HCl (36.5-38.0%) to 917 mL of distilled or deionized water. Work in a fume hood and use proper protective gear. This reagent may be stored at room temperature for 2 years.

Sample Preparation


Sample extraction protocols are to be designed and validated by the individual users of this kit. The following suggestions are guidelines, and define the manner in which the kit is performance tested by the manufacturer.



Obtain Samples, Extract

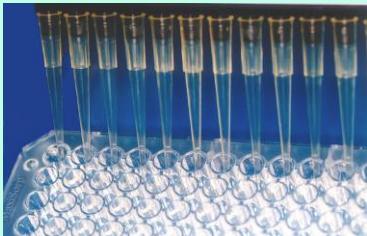

Add Conjugate, Control, and sample extract

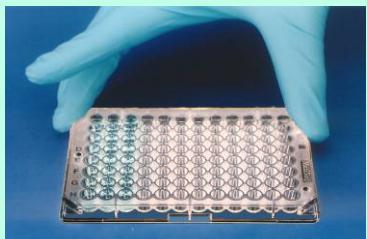

Mix plate



Incubate



Wash

1. Green leaf samples: Extract green corn or cotton leaf samples that are 5-10 mm² in size with **250 µL** of **Extraction Buffer**. The extraction efficiency will vary proportionately with the amount of tissue disruption performed. *Use extreme caution to prevent sample-to-sample cross-contamination with plant tissue or exudate.* Allow solids to settle before transferring extract to the assay plate. Dispensing particles into the assay plate can cause false positive results.
2. Single seed samples: Crush corn kernels or cotton seeds and extract each with **1 mL** of **Extraction Buffer**. Allow solids to settle before transferring extract to the assay plate. Dispensing particles into the assay plate can cause false positive results.

How to Run the Assay

- Read all of these instructions before running the kit.
- Allow all reagents to reach room temperature before beginning (at least 30 minutes with un-boxed strips and reagents at room temperature - do not remove strips from bag with desiccant until they have warmed up).
- Organize all reagents, sample extracts, and pipettes so that step 1 can be performed in 15 minutes or less. The use of a multichannel pipette may be needed to adhere to this time constraint.
- Use a disposable-tip air-displacement pipette and a clean pipette tip to add Blank, Positive Control, and sample extract to the wells. Conjugate, Substrate, and Stop Solution may be added in the same manner; alternatively, use a repeating pipette with a disposable tip on the end of the Combitip for these three reagents.
- Use the well identification markings on the plate frame to guide you when adding the samples and reagents. It is recommended that at least two wells each of Blank (Extraction Buffer) and Cry2A Positive Control be run on each plate. Additional quality control samples may be added at the discretion of the user. Sample extracts may be run in either single or duplicate wells.

Procedure

1. Add **50 µL** of **Cry2A Enzyme-Conjugate** to each well of the plate. Immediately follow with **50 µL** of Extraction Buffer **Blank**, **50 µL** of **Cry2A Positive Control**, and **50 µL** of each **user-supplied control/sample extract** to their respective wells. Follow this same order of addition for all reagents.

NOTE: In order to minimize setup time it is recommended that a multi-channel pipette be used in steps 1, 5 and 7 when more than 4 strips are used.

2. Thoroughly mix the contents of the wells by moving the strip holder in a rapid circular motion on the benchtop for a full 20-30 seconds. Be careful not to spill the contents!
3. Cover the wells with tape or Parafilm to prevent evaporation and **incubate at ambient temperature for 45 minutes**. If an orbital plate shaker is available shake plate at 200 rpm. (Alternate timing steps may be used with this kit; please consult EnviroLogix Tech Support.)
4. After incubation, carefully remove the covering and vigorously shake the contents of the wells into a sink or other suitable container. Flood the wells completely with **Wash Buffer**, then shake to empty. Repeat this wash step



Read plates in a Plate Reader within 30 minutes of the addition of Stop Solution

Precautions and Notes

- *Store all Kit components at 4°C to 8°C (39°F to 46°F) when not in use.*
- *Do not expose Kit components to temperatures greater than 37°C (99°F) or less than 2°C (36°F).*
- *Allow all reagents to reach ambient temperature (18°C to 27°C or 64°F to 81°F) before use.*
- *Do not use kit components after the expiration date.*
- *Do not use reagents or test well strips from one Kit with reagents or test well strips from a different Kit.*
- *Do not expose Substrate to sunlight during pipetting or while incubating in the test wells.*
- *The assay has been optimized for use with the protocol provided in the kit. Deviation from this protocol may invalidate the results of the test.*
- *As with all tests, it is recommended that results be confirmed by an alternate method when necessary.*
- *Cry2A endotoxins are proteins which can be degraded by heat and sunlight. Take samples from green, actively growing leaves. Samples that cannot be extracted immediately may be stored frozen for up to 1 week prior to analysis.*
- *Observe any applicable regulations when disposing of samples and kit reagents.*

three times, for a total of 4 washes. Slap the plate on a paper towel to remove as much water as possible. Alternatively, perform these four washes with a microtiter plate or strip washer set for sequential 300 µL fill/aspirate cycles.

5. Add **100 µL** of **Substrate** to each well.
6. Thoroughly mix the contents of the wells, as in step 2. Cover the wells with new tape or Parafilm and incubate **for 15 minutes** at ambient temperature. Use orbital shaker if available. (NOTE: Alternate timing steps may be used with this kit; please consult EnviroLogix Tech Support.)

Caution: Stop Solution is 1.0N Hydrochloric acid. Handle carefully.

7. Add **100 µL** of **Stop Solution** to each well and mix thoroughly. This will turn the well contents yellow.

NOTE: Read the plate within 30 minutes of the addition of Stop Solution.

How to Interpret the Results

Spectrophotometric Measurement

1. Set the wavelength of your microtiter plate reader to 450 nanometers (nm). (If it has dual wavelength capability, use 600, 630 or 650 nm as the reference wavelength.)
2. Set the plate reader to blank on the Extraction Buffer **Blank** wells. If the reader cannot do this, measure and record the optical density (OD) of each well's contents, then subtract the average OD of the **Blank** wells from each of the readings.

General test criteria:

The mean OD of the BLANK wells should not exceed 0.15.

The mean, blank-subtracted OD of the Positive Control wells should be at least 0.2.

The coefficient of variance (%CV) between the duplicate Positive Control wells should not exceed 15%:

$$\%CV = \frac{\text{std. deviation of OD's}}{\text{mean Pos.Ctl. OD}} \times 100$$

If the results of an assay fail to meet these criteria, consult EnviroLogix' Technical Service for suggestions on improving the test when you repeat the assay.

Calculate the Positive Control Ratio

Divide the OD of each sample extract by the mean OD of the Positive Control wells. This number is the "Positive Control Ratio".

Interpret the Qualitative Results

Single Corn or Cotton Leaf and Seed samples:

If the Positive Control Ratio calculated for a sample is less than 1.0, the sample does not contain Cry2A protein.

If the Positive Control Ratio of a sample is greater than or equal to 1.0, the sample does contain Cry2A protein.

Leaf and seed samples are by their nature either 100% positive or 100% negative. Any low level positive results from single seed or leaf samples must be due to either some form of sample cross-contamination (stray particles or dust from Event 603 corn or cotton, leaf residue on leaf punch, etc.) or can be caused by transfer of particulate matter from leaf or seed extracts into the assay wells. If there is any question of the latter occurring, re-extraction and re-testing is recommended.

Figure 1A. Example of a typical Qualitative assay setup.

	1	2	3	4	5	6	7	8	9	10	11	12
A	BL	S7	S15	S23	S31	S39	S47	S55	S63	S71	S79	S87
B	PC	S8	S16	S24	S32	S40	S48	S56	S64	S72	S80	S88
C	S1	S9	S17	S25	S33	S41	S49	S57	S65	S73	S81	S89
D	S2	S10	S18	S26	S34	S42	S50	S58	S66	S74	S82	S90
E	S3	S11	S19	S27	S35	S43	S51	S59	S67	S75	S83	S91
F	S4	S12	S20	S28	S36	S44	S52	S60	S68	S76	S84	S92
G	S5	S13	S21	S29	S37	S45	S53	S61	S69	S77	S85	BL
H	S6	S14	S22	S30	S38	S46	S54	S62	S70	S78	S86	PC

“BL” = Blank wells (Extraction Buffer)

“PC” = Cry2A Positive Control Wells

“S..” = sample extracts



LIMITED WARRANTY

EnviroLogix Inc. ("EnviroLogix") warrants the products sold hereunder ("the Products") against defects in materials and workmanship when used in accordance with the applicable instructions for a period not to extend beyond a product's printed expiration date. If the Products do not conform to this Limited Warranty and the customer notifies EnviroLogix in writing of such defects during the warranty period, including an offer by the customer to return the Products to EnviroLogix for evaluation, EnviroLogix will repair or replace, at its option, any product or part thereof that proves defective in materials or workmanship within the warranty period.

ENVIROLOGIX MAKES NO OTHER WARRANTIES, EXPRESSED OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. The warranty provided herein and the data, specifications and descriptions of EnviroLogix products appearing in EnviroLogix published catalogues and product literature are EnviroLogix' sole representations concerning the Products and warranty. No other statements or representations, written or oral, by EnviroLogix' employees, agents or representatives, except written statements signed by a duly authorized officer of EnviroLogix Inc., are authorized; they should not be relied upon by the customer and are not a part of the contract of sale or of this warranty.

EnviroLogix does not warrant against damages or defects arising in shipping or handling, or out of accident or improper or abnormal use of the Products; against defects in products or components not manufactured by EnviroLogix, or against damages resulting from such non-EnviroLogix made products or components. EnviroLogix passes on to customer the warranty it received (if any) from the maker thereof of such non-EnviroLogix made products or components. This warranty also does not apply to Products to which changes or modifications have been made or attempted by persons other than pursuant to written authorization by EnviroLogix.

THIS WARRANTY IS EXCLUSIVE. The sole and exclusive obligation of EnviroLogix shall be to repair or replace the defective Products in the manner and for the period provided above. EnviroLogix shall not have any other obligation with respect to the Products or any part thereof, whether based on contract, tort, strict liability or otherwise. Under no circumstances, whether based on this Limited Warranty or otherwise, shall EnviroLogix be liable for incidental, special, or consequential damages.

This Limited Warranty states the entire obligation of EnviroLogix with respect to the Products. If any part of this Limited Warranty is determined to be void or illegal, the remainder shall remain in full force and effect.

*Parafilm is a registered trademark of American Can Corporation
EnviroLogix, the EnviroLogix logo and QuantiPlate are trademarks
of EnviroLogix Inc.*

© EnviroLogix 2009

