

Highlights:

- Results in 5 minutes or less
- Both bulk soybean kits utilize Common Extraction™:
 - Roundup Ready®
 - LibertyLink®
- Available as 100-strip kit, in bulk packaging, or in QuickCombs™

Contents of Kit:

- 100 QuickStix Strips packed in two moisture-resistant canisters
- 100 transfer pipettes
- 100 three-ounce cups

Items Not Provided:

- Blender for sample prep:
 1. Oster® Sunbeam blender model #4094 (with 4 oz. polystyrene blender jar, ice crusher blade, gasket, and blender base) ~or~
 2. Waring blender model 31BL91 or equivalent (with glass Mason jars and jar adapter [Eberbach #E8495] along with protective cover ~or~
 3. BUNN coffee grinder (industrial style grinder set on AutoDrip setting)
- Graduated cylinder
- Tap water
- Protective cover for blender jar while grinding
- QuickScan System (optional, for quantitative results)

Catalog Number AQ 010 BGB

Intended Use

This EnviroLogix QuickStix Kit for QuickScan - Roundup Ready Bulk Soybeans is designed to extract and detect the presence of CP4 EPSPS protein at the levels typically expressed in Roundup Ready soybeans. The sensitivity of these QuickStix Strips is 0.25% Roundup Ready soybean (i.e. one Roundup Ready soybean in 400 conventional soybeans).

How the Test Works

In order to detect the CP4 EPSPS protein expressed by Roundup Ready soybeans, the sample must first be extracted to solubilize the protein. Each QuickStix Strip has an absorbent pad at each end. The protective tape with the arrow indicates the end of the strip to insert into the reaction cup. The sample will travel up the membrane strip and be absorbed into the larger pad at the top of the strip. The portion of the strip between the protective tape and the absorbent pad at the top of the strip is used to view the reactions as described under “Interpreting the Results.” Results may then be scanned and interpreted quantitatively with the EnviroLogix QuickScan System. Please avoid bending the strips.

Sample Preparation

Step 1: Determine Number and Size of Sub-samples

1. Collect a composite sample according to USDA/ GIPSA instructions found in the following reference documents:
 - <http://archive.gipsa.usda.gov/reference-library/handbooks/grain-insp/grbook1/bk1.pdf> - USDA Grain Inspection Handbook, Book 1, Grain Sampling.
 - <http://archive.gipsa.usda.gov/biotech/sample2.htm> - Guidance document entitled Sampling for the Detection of Biotech Grains.
 - <http://archive.gipsa.usda.gov/biotech/sample1.htm> - Practical Application of Sampling for the Detection of Biotech Grains.
 - <http://archive.gipsa.usda.gov/biotech/samplingplan1.xls> - This website provides a simple to use Sample Planner (29K Excel Spreadsheet). The planner allows you to enter different assumptions in terms of sample size, number of samples, acceptable quality level and to determine the probability of accepting lots with given concentration levels. It also plots the probabilities in graph form for easy interpretation. Specific data can be saved for documentation and future analyses.
2. The following is a helpful reference for use in designing a sampling plan: Remund, K.M., Dixon, D.A., Wright D.L., Holden, L.R. “Statistical considerations in seed purity testing for transgenic traits”, Seed Science Research, June 2001, Vol. 11 No.2, pp. 101-119.

- To select the appropriate sample size, determine the purity standard and the degree of confidence required. Confidence level means the statistical probability that the true Roundup Ready level in the lot is below the selected purity standard. Table 1 provides a guideline for determining the number of 400 bean subsamples that are necessary to provide effective screening for different GM concentrations at a 95% confidence level.

Table 1 - Number of 400 soybean subsamples required for testing

Confidence Level (%)	Roundup Ready Soybean Screening Level	
	0.5 %	0.25%
95%	2	3

For other sampling scenarios or different screening or confidence levels, refer to the USDA/GIPSA Excel spreadsheet described under Step 1 above, or call EnviroLogix Technical Support for assistance.

Step 2: Determine Sub-sample Weight, Jar Size and Grind Times

- Determine average weight of individual grain to be tested (weigh 100 beans, divide by 100).
- Calculate the weight of the number of grains to be tested (Number of grains X Average Weight/Grain). Table 2 lists the guidelines for jar size and grinding time according to sample weight.
- Choose an appropriate jar size and grind time based on the type of blender available for sub-sample preparation (see Table 2). Oster Sunbeam Blender with ice crusher blade is recommended over the Waring Blender for its bean grinding efficiency. (Note that bean grind time is longer and requires additional steps* when using a Waring Blender).

Table 2 - Soybeans

# of Beans (approximate)	Blender Type	Sub-sample weight (g)	Jar size (oz.)	Grind Time on High Speed
100-200	Oster Sunbeam	16-38	8	20 seconds
100	Waring	16-38	8	60 seconds (2 X 30 sec.*)
200-400	Waring	38-65	16	60 seconds (2 X 30 sec.*)

* For best results blend beans for 1/2 of total time, remove the jar and shake to redistribute larger particles, replace and resume grinding.

- Choose an appropriate jar size for the sample based upon Table 2 above.

Step 3: Prepare the Sample

- Weigh sample into the appropriate vessel.
- Put protective cover over glass jars.
- Grind sample on high speed until all whole beans are finely ground.
- Add the volume of tap water calculated by the formula (left).



Choose grinding method

Soybean Common Extraction

Grams of beans x 5 = mL water
 For example: (100 x 0.15)=15g
 15 g x 5 = 75 mL water

Extract in tap water



Transfer extract to cup, about 3 pipettefuls

5. Cap and shake jar vigorously until the entire sample is wet (20-30 seconds, depending on the number of grains). Sample will begin to settle immediately and liquid can be drawn off at that time. Avoid pulling up particles with the transfer pipette.
6. Transfer 12 mL of the liquid extract from above the settled soybean solids into the three-ounce sample cup. The level of extract should be above the bottom of the arrow tape yet below the top of the arrow on the bottom portion of the strip.
7. To prevent cross-contamination thoroughly clean blender parts and jars of dust and residue prior to preparation of a second sample. Use a new transfer pipette and cup for each sample.

How to Run the QuickStix Strip Test

1. Allow refrigerated canisters to come to room temperature before opening. Remove the QuickStix Strips to be used. Avoid bending the strips. Reseal the canister immediately.
2. Place the strip into the three-ounce cup containing 12 mL of the liquid soybean extract. The sample will travel up the strip.
3. Allow the strip to develop for 5 minutes before making final assay interpretations. Positive sample results may become obvious much more quickly.
4. To retain the strip, or for use in the QuickScan System, cut off and discard the bottom section of the strip covered by the arrow tape.

NOTE: Use extreme caution to prevent sample-to-sample cross-contamination with grain, fluids, or disposables.

Interpreting the Results

Development of the Control Line within 5 minutes indicates that the strip has functioned properly. Any strip that does not develop a Control Line should be discarded, and the sample re-tested using another strip.

If the extract is from a sample containing at least 0.25% Roundup Ready soybean (1 in 400), a second line (Test Line) will develop on the membrane strip between the Control Line and the protective tape. *The results should be interpreted as positive for CP4 EPSPS protein expression.*

If the extract is from a negative sample, the strip will only show the control line.


Results may then be scanned and interpreted quantitatively with the QuickScan System. Please consult the QuickScan User Manual for details.

Kit Storage

QuickStix can be stored at room temperature, or refrigerated for a longer shelf life. Note the shelf life on the kit box for each storage temperature. The kit may be used in field applications; however, prolonged exposure to high temperatures may adversely affect the test results. Do not open the desiccated canister until ready to use the test strips.



Any clearly discernable pink Test Line is considered positive

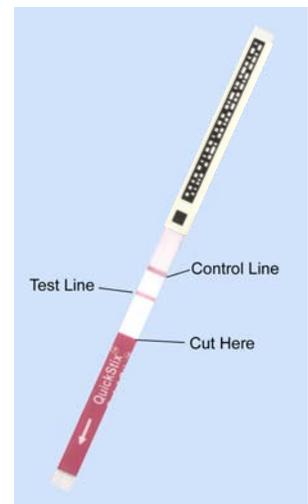

Precautions and Notes

- This kit is designed to be read visually as a screen for presence or absence, and is also designed to be quantitative when used with the QuickScan System.
- This product is currently not applicable for use in any other crop or in leaf or individual seed testing.
- As with all tests, it is recommended that results be confirmed by an alternate method when necessary.
- The assay has been optimized to be used with the protocol provided in the kit. Deviation from this protocol may invalidate the results of the test.
- The results generated through the proper use of this diagnostic tool reflect the condition of the working sample directly tested. Extrapolation as to the condition of the originating lot, from which the working sample was derived, should be based on sound sampling procedures and statistical calculations which address random sampling effects, non-random seed lot sampling effects and assay system uncertainty. A negative result obtained when properly testing the working sample does not necessarily mean the originating lot is entirely negative for the analyte or protein in question.
- A strong positive result may safely be interpreted in as little as 2 minutes after sample addition. It is not safe, however, to interpret negative results prior to 5 minutes.
- Protect all components from hot or cold extremes of temperature when not in use.
- **CAUTION:** Tightly closed containers of soy extract, if left sitting for several hours, may ferment and cause the lid or container to burst. Dispose of extract when testing is complete.





**For Technical Support
Contact Us At:**

EnviroLogix
500 Riverside Industrial
Parkway
Portland, ME 04103-1486
USA

Tel: (207) 797-0300
Toll Free: 866-408-4597
Fax: (207) 797-7533

e-mail:
info@envirologix.com

website:
www.envirologix.com



LIMITED WARRANTY

EnviroLogix Inc. ("EnviroLogix") warrants the products sold hereunder ("the Products") against defects in materials and workmanship when used in accordance with the applicable instructions for a period not to extend beyond a product's printed expiration date. If the Products do not conform to this Limited Warranty and the customer notifies EnviroLogix in writing of such defects during the warranty period, including an offer by the customer to return the Products to EnviroLogix for evaluation, EnviroLogix will repair or replace, at its option, any product or part thereof that proves defective in materials or workmanship within the warranty period.

NEITHER ENVIROLOGIX NOR MONSANTO MAKES ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. The warranty provided herein and the data, specifications and descriptions of EnviroLogix products appearing in EnviroLogix published catalogues and product literature are EnviroLogix' sole representations concerning the Products and warranty. No other statements or representations, written or oral, by EnviroLogix' employees, agents or representatives, except written statements signed by a duly authorized officer of EnviroLogix Inc., are authorized; they should not be relied upon by the customer and are not a part of the contract of sale or of this warranty.

EnviroLogix does not warrant against damages or defects arising in shipping or handling, or out of accident or improper or abnormal use of the Products; against defects in products or components not manufactured by EnviroLogix, or against damages resulting from such non-EnviroLogix made products or components. EnviroLogix passes on to customer the warranty it received (if any) from the maker thereof of such non-EnviroLogix made products or components. This warranty also does not apply to Products to which changes or modifications have been made or attempted by persons other than pursuant to written authorization by EnviroLogix.

THIS WARRANTY IS EXCLUSIVE. The sole and exclusive obligation of EnviroLogix shall be to repair or replace the defective Products in the manner and for the period provided above. EnviroLogix shall not have any other obligation with respect to the Products or any part thereof, whether based on contract, tort, strict liability or otherwise. Under no circumstances, whether based on this Limited Warranty or otherwise, shall EnviroLogix be liable for incidental, special, or consequential damages.

This Limited Warranty states the entire obligation of EnviroLogix with respect to the Products. If any part of this Limited Warranty is determined to be void or illegal, the remainder shall remain in full force and effect.

License

EnviroLogix has developed this kit using proprietary reagents as well as reagents licensed from Monsanto Company.

*Roundup Ready is a registered trademark of Monsanto Technology, LLC
EnviroLogix, the EnviroLogix logo, QuickStix, QuickScan, and Common Extraction are trademarks of EnviroLogix Inc.*

© EnviroLogix 2009